



填写部门	检验员
保存年限	五年

## 一次性口罩成品检验报告

### Test report of disposable face masks

报告日期: 2020年05月25日

Report Date: 2020.05.25

检验依据: GB T32610-2016 《日常防护型口罩技术规范》


Test basis: GB T32610-2016 Technical specification for daily protective masks

规格: 17.5cm×9.5cm 生产数量: 2000000 抽检数量: 50 生产批号: GK20412 订单号: GK20425  
 Size: 17.5cm×9.5cm Quantity: 2000000PCS Amount Tested: 50PCS LOT : GK20412 Order#: GK20425

检验项目 Test Item	条款 Terms	性能指标 Standard Requirements	检验结果 Test Result	结论 Conclusion
基础要求 Basic requirements	1.1	口罩应能安全牢固地护住口、鼻。 The mask should be able to protect the mouth and nose safely and firmly.	符合 Pass	合格 Qualified
	1.2	口罩原材料不应使用再生料, 无异味。 The raw materials of the masks should not use recycled materials and have no peculiar smell.	符合 Pass	合格 Qualified
	1.3	口罩不应存在可触及的锐利角和锐利边缘, 不对佩戴者构成伤害。 There should be no sharp angles and sharp edges that can be touched by the mask, which should not cause harm to the wearer.	符合 Pass	合格 Qualified
	1.4	口罩应便于佩戴和摘除, 在佩戴过程中无明显的压迫感或压痛现象, 对头部活动影响较小。 The mask should be easy to put on and take off. There is no obvious feeling of pressure or tenderness during wearing, which has little effect on head movement.	符合 Pass	合格 Qualified
外观 Appearance	2.1	口罩表面不应有破损、油污斑渍\变形及其他明显的缺陷。 The surface of the mask should not be damaged, stained, deformed and other obvious defects.	符合 Pass	合格 Qualified
规格尺寸 Size	3.1	尺寸 17.5×9.5cm 注: 尺寸允许误差±0.5cm。 Size: 17.5cm×9.5cm Note: Tolerance ±0.5cm	17.5×9.5	合格 Qualified
鼻夹 Nose clip	4.1	口罩上应配有鼻夹, 鼻夹长度应不小于8cm。 The nose mask should be equipped with a nose clip, the length of the nose clip should not be less than 8cm.	9CM	合格 Qualified
口罩带 Mask strap	5.1	每根口罩带与口罩体连接点处的断裂强力应不小于10N。 The breaking strength at the connection point between each mask strap and mask should not be less than 10N.	>10N	合格 Qualified
微生物清洁度 (cfu/g) Microbial cleanliness	6.1	≤30	12	TYPE I
压力差 (pa/cm <sup>2</sup> ) Differential pressure	7.1	<40	25	TYPE I
抗溅压力 (kPa) Splash resistance pressure	8.1	≥16.0	≥16	TYPE I
细菌过滤 (BFE) % Bacterial filtration efficiency (BFE)	9.1	≥95%	96.25	TYPE I
备注 Remarks	11.1	附照片, 附件一。 Attached photo in Annex		
检验结论 Test conclusion :	经检验的产品样本各项指标均符合 GB T32610-2016 《日常防护型口罩技术规范》 All indexes of the tested product samples meet the requirements in GB T32610-2016 Technical specification for daily protective masks			

检验人/Test: 曹璐

审核人/Check: 许丽

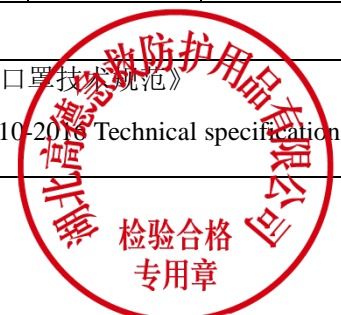





## Mask Instructions Instructions pour le masque

DONNING A MASK  
COMMENT ENFILER UN MASQUE



DOFFING A MASK  
COMMENT ENLEVER UN MASQUE



1 800 221-0222 | English: [mpm@redcross.ca](mailto:mpm@redcross.ca) | Français: [msc@croisiered.org](mailto:msc@croisiered.org)

